



InertSearch™ for LC

Inertsil® Applications

Analysis of Sitagliptin

(Under the Condition of draft for USP, Sitagliptin and Metformin Hydrochloride Tablets)

Data No. LB548-0812

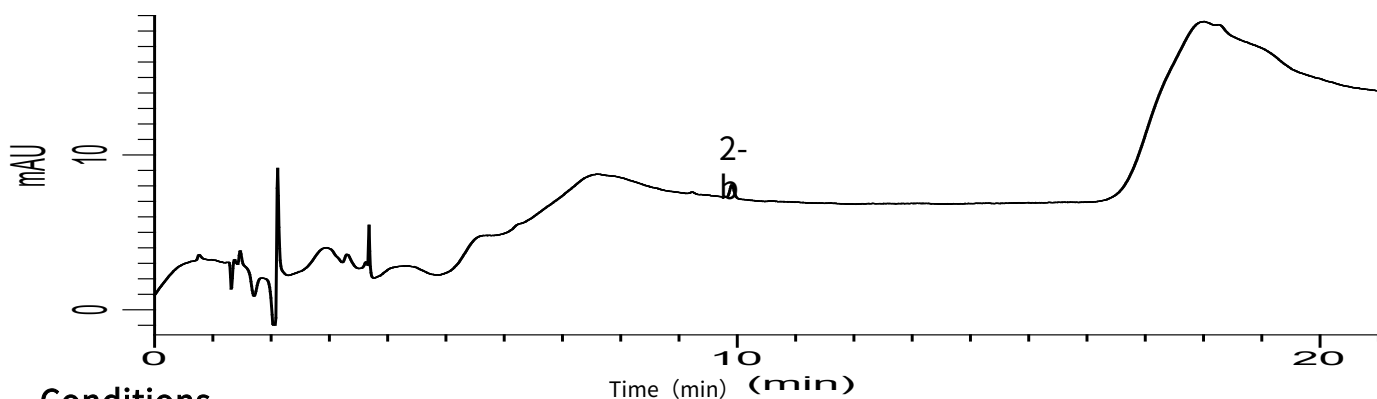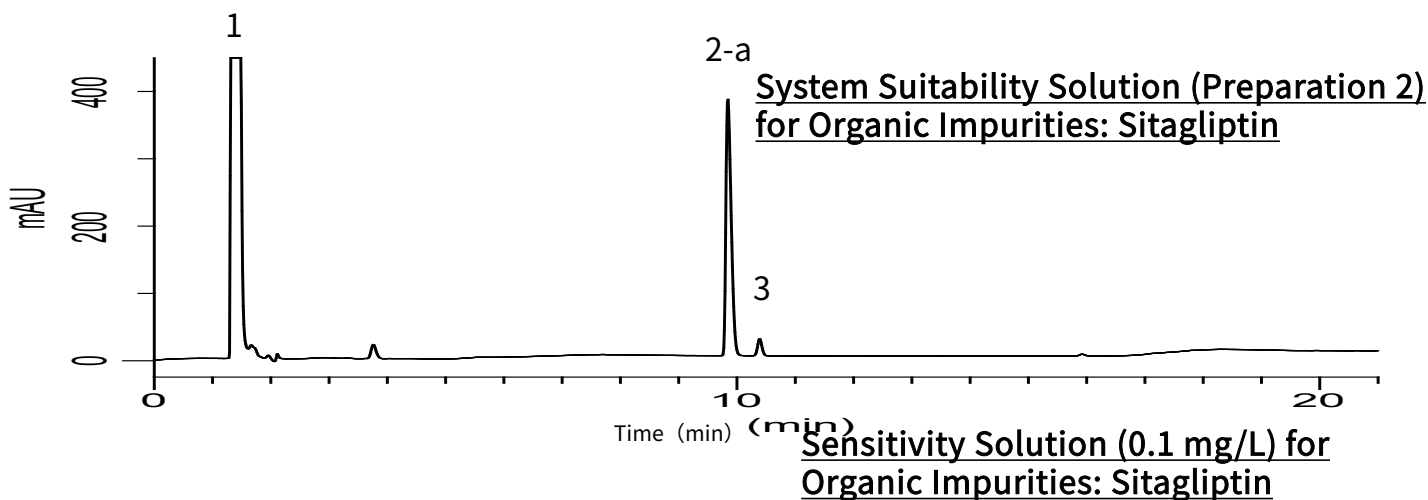

Conditions

System : GL7700 HPLC system
Column : InertSustain C18 (3 µm HP, 150 x 4.6 mm I.D.)
Column Cat. No. : 5020-14445
Eluent : A) CH₃CN
 : B) CH₃CN/Buffer* = 5/95, v/v

Analyte:

1. Metformin
2. Sitagliptin
3. Fumarate adduct of Sitagliptin

Resolution (2-a, 3) : 3.40 (> 1.5)
S/N for 2-b : 40.0 (> 10)

Time (min)	A (vol%)	B (vol%)
0	13	87
2	13	87
21	47	53
21.01	13	87
25	13	87

Flow rate : 1.0 mL/min
Col. Temp. : 40 °C
Detection : UV 205 nm (UV7750 UV Detector)
Injection Vol. : 20 µL
Sample : Standard

* 3.45 g/L of monobasic sodium phosphate (0.025 M). Adjust with phosphoric acid to a pH of 2.5.